




J DENTAL CARE

just smile

JD ICON PLUS

Bone tissue implant system



conical connection



Made in Italy

BONE TISSUE IMPLANT SYSTEM


ONE CONNECTION for all sizes of fixtures and a simplified restorative workflow

EXCELLENT PRIMARY STABILITY, ideal for immediate loading.


COMPLETE RANGE OF PROSTHETIC OPTIONS from single element to full-arch restorations

LONGER IMPLANTS (18-30 mm) available to solve the most challenging cases even in atrophic maxilla.

FRictional MORSE TAPER CONNECTION

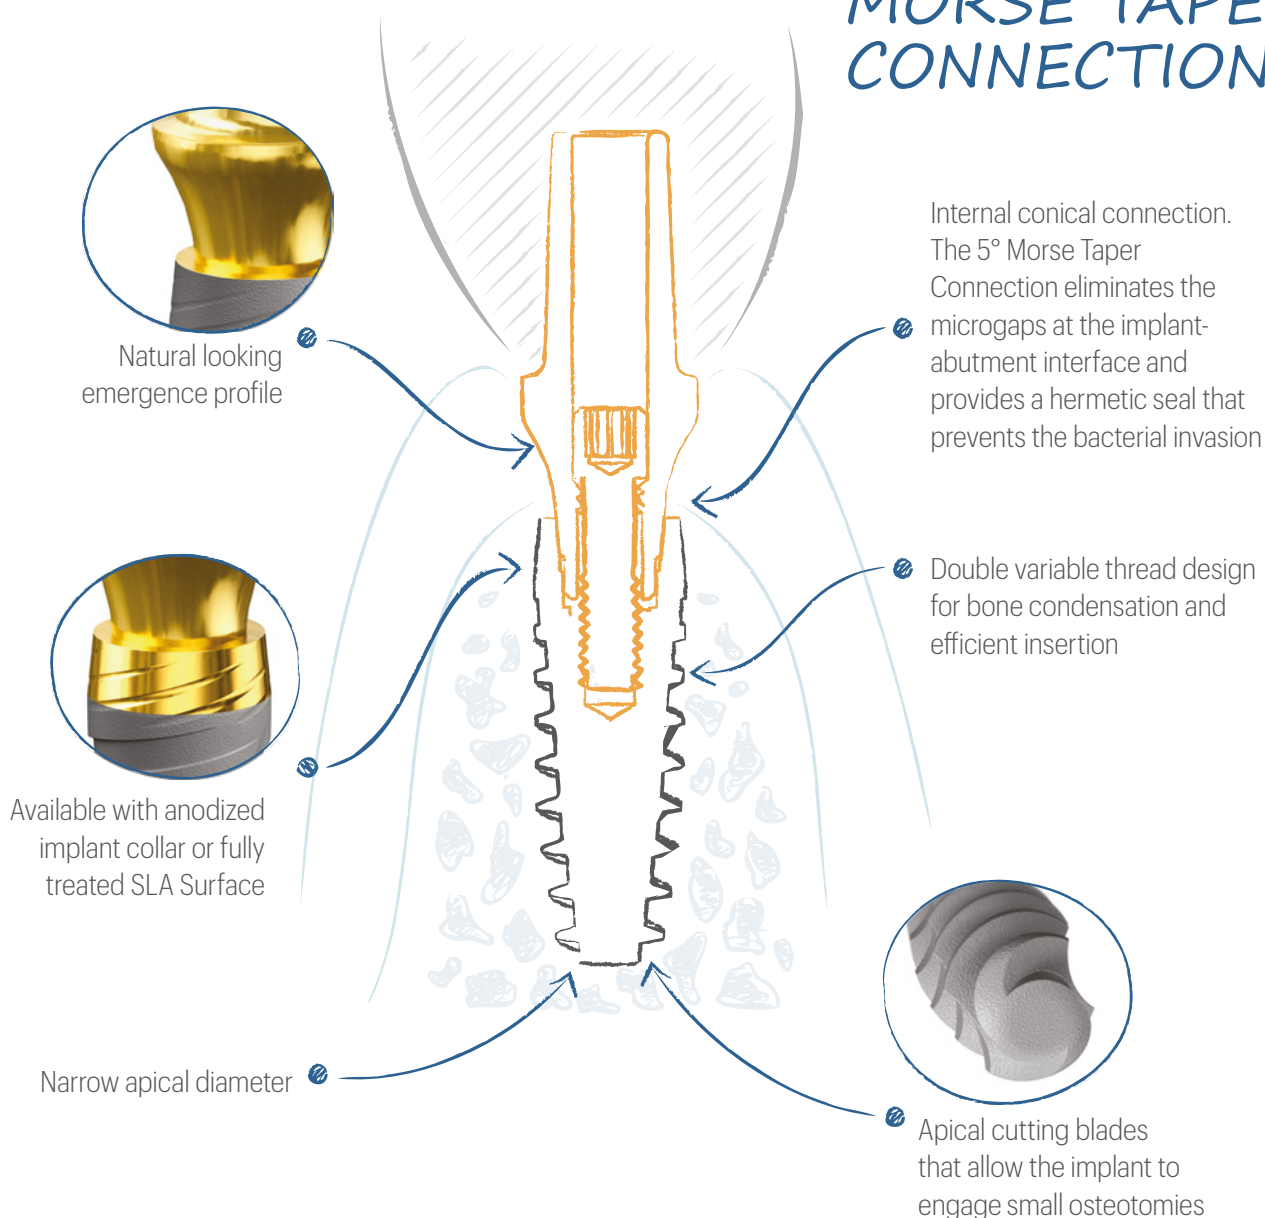

BONE TISSUE SURFACE TREATMENT

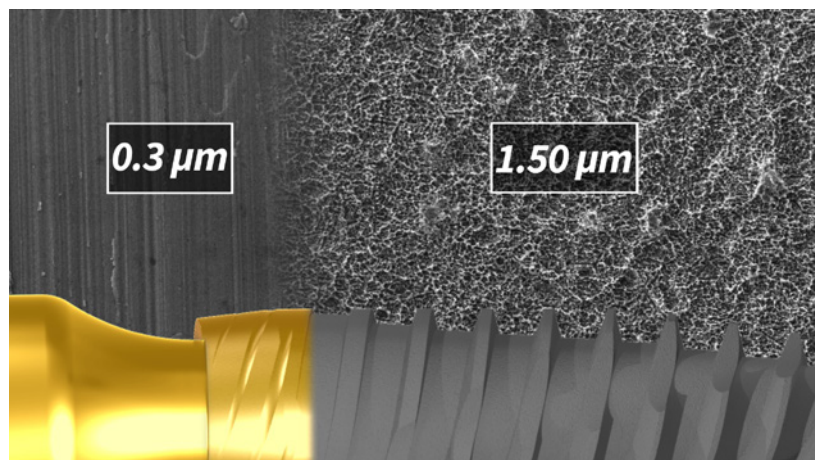

The JDIcon Plus dental implants are available in two versions:


1. Fully treated with SLA surface treatment
2. With anodized implant collar and body surface treated with SLA

The S.L.A. surface is obtained through the procedure of sandblasting with large grit and acid-etching (SLA) which guarantees an optimal microtopography of the implant surface that improves the osteointegration.

Note: The picture above is generated by a Scanning electron microscope (SEM) and shows the roughness values, expressed as Ra, of the two surfaces of the implant treated with S.L.A. and Anodization.

PRODUCT SPECIFICATIONS

IMPLANT DIAMETER	LENGTH	TIP DIAMETER	PLATFORM DIAMETER	ABUTMENT INTERFACE
JDIcon Plus				
Ø 3,7	8	2.8	3.7	3.1
	10, 11.5, 13, 15, 18	2.4		
Ø 4,3	6	2.4	3.8	3.1
	8	3.2	4	
	10, 11.5, 13, 15, 18	2.8		
Ø 5,0	6	2.8	4.7	3.1
	8	3.2	4.8	
	10, 11.5, 13			
JDIcon Plus PT				
Ø 4,0	13, 15, 18, 20	2.4	4.0	3.1
JDIcon Plus LE				
Ø 4,0	18, 20, 22, 24, 26, 28, 30	2.4	4.0	3.1

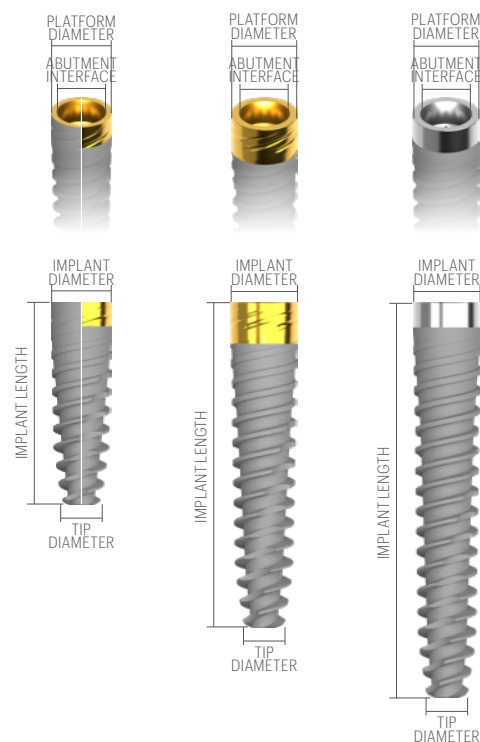

PRODUCT CATALOGUE

Note: all measurements of diameters and lengths are in mm

JDIcon Plus:


Ø 3,7

IC37080.	JDIcon Plus Ø 3,7 L 8
IC37100.	JDIcon Plus Ø 3,7 L 10
IC37115.	JDIcon Plus Ø 3,7 L 11,5
IC37130.	JDIcon Plus Ø 3,7 L 13
IC37150.	JDIcon Plus Ø 3,7 L 15
IC37180.	JDIcon Plus Ø 3,7 L 18




Ø 4,3

IC43060.	JDIcon Plus Ø 4,3 L 6
IC43080.	JDIcon Plus Ø 4,3 L 8
IC43100.	JDIcon Plus Ø 4,3 L 10
IC43115.	JDIcon Plus Ø 4,3 L 11,5
IC43130.	JDIcon Plus Ø 4,3 L 13
IC43150.	JDIcon Plus Ø 4,3 L 15
IC43180.	JDIcon Plus Ø 4,3 L 18

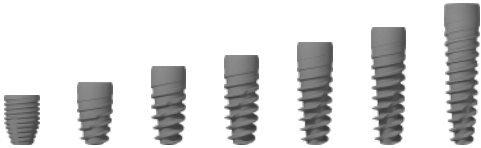

Ø 5,0

IC50060.	JDIcon Plus Ø 5,0 L 6
IC50080.	JDIcon Plus Ø 5,0 L 8
IC50100.	JDIcon Plus Ø 5,0 L 10
IC50115.	JDIcon Plus Ø 5,0 L 11,5
IC50130.	JDIcon Plus Ø 5,0 L 13



JDIcon Plus (anodised collar):


Ø 3,7

IC37080,	JDIcon Plus Anodized Collar Ø 3,7 L 8
IC37100,	JDIcon Plus Anodized Collar Ø 3,7 L 10
IC37115,	JDIcon Plus Anodized Collar Ø 3,7 L 11,5
IC37130,	JDIcon Plus Anodized Collar Ø 3,7 L 13
IC37150,	JDIcon Plus Anodized Collar Ø 3,7 L 15
IC37180,	JDIcon Plus Anodized Collar Ø 3,7 L 18



Ø 4,3

IC43060,	JDIcon Plus Anodized Collar Ø 4,3 L 6
IC43080,	JDIcon Plus Anodized Collar Ø 4,3 L 8
IC43100,	JDIcon Plus Anodized Collar Ø 4,3 L 10
IC43115,	JDIcon Plus Anodized Collar Ø 4,3 L 11,5
IC43130,	JDIcon Plus Anodized Collar Ø 4,3 L 13
IC43150,	JDIcon Plus Anodized Collar Ø 4,3 L 15
IC43180,	JDIcon Plus Anodized Collar Ø 4,3 L 18

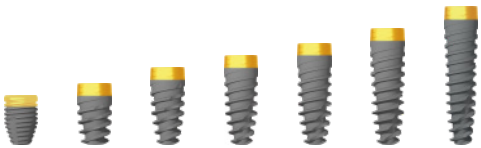


Ø 5,0

IC50060,	JDIcon Plus Anodized Collar Ø 5,0 L 6
IC50080,	JDIcon Plus Anodized Collar Ø 5,0 L 8
IC50100,	JDIcon Plus Anodized Collar Ø 5,0 L 10
IC50115,	JDIcon Plus Anodized Collar Ø 5,0 L 11,5
IC50130,	JDIcon Plus Anodized Collar Ø 5,0 L 13



JDIcon Plus PT:

ICPT40130.	JDIcon Plus PT Ø 4.0 L 13
ICPT40150.	JDIcon Plus PT Ø 4.0 L 15
ICPT40180.	JDIcon Plus PT Ø 4.0 L 18
ICPT40200.	JDIcon Plus PT Ø 4.0 L 20



JDIcon Plus LE:

ICNAE40180.	JDIcon Plus LE Ø 4.0 L 18
ICNAE40200.	JDIcon Plus LE Ø 4.0 L 20
ICNAE40220.	JDIcon Plus LE Ø 4.0 L 22
ICNAE40240.	JDIcon Plus LE Ø 4.0 L 24
ICNAE40260.	JDIcon Plus LE Ø 4.0 L 26
ICNAE40280.	JDIcon Plus LE Ø 4.0 L 28
ICNAE40300.	JDIcon Plus LE Ø 4.0 L 30



Cover screw:

ICCS. Cover Screw JDIcon Plus



Healing Abutment:

ICHA43. Healing Abutment Ø 4.0 H 3.0 JDIcon Plus
 ICHA45. Healing Abutment Ø 4.0 H 5.0 JDIcon Plus
 ICHA47. Healing Abutment Ø 4.0 H 7.0 JDIcon Plus
 ICHA53. Healing Abutment Ø 5.0 H 3.0 JDIcon Plus
 ICHA55. Healing Abutment Ø 5.0 H 5.0 JDIcon Plus
 ICHA57. Healing Abutment Ø 5.0 H 7.0 JDIcon Plus
 ICHA63. Healing Abutment Ø 6.0 H 3.0 JDIcon Plus
 ICHA65. Healing Abutment Ø 6.0 H 5.0 JDIcon Plus
 ICHA67. Healing Abutment Ø 6.0 H 7.0 JDIcon Plus
 ICHA753. Healing Abutment Ø 7.5 H 3.0 JDIcon Plus
 ICHA755. Healing Abutment Ø 7.5 H 5.0 JDIcon Plus



Impression Coping:

OPEN TRAY

ICICOT4C. Impression Coping Open Tray Ø 4.0 JDIcon Plus
 ICICOT5C. Impression Coping Open Tray Ø 5.0 JDIcon Plus
 ICICOT6C. Impression Coping Open Tray Ø 6.0 JDIcon Plus
 ICICOTS. Impression Coping Open Tray Screw JDIcon Plus



CLOSED TRAY

ICICCT4C. Impression Coping Closed Tray Ø 4.0 JDIcon Plus
 ICICCT5C. Impression Coping Closed Tray Ø 5.0 JDIcon Plus
 ICICCT6C. Impression Coping Closed Tray Ø 6.0 JDIcon Plus
 ICICCT1C. Impression Coping Closed Tray Direct Press Fit JDIcon Plus
 ICICCTS. Impression Coping Closed Tray Screw JDIcon Plus



Temporary Abutment:

ICTAEC. Temporary Abutment Engaging JDIcon Plus
 ICTANEC. Temporary Abutment Non Engaging JDIcon Plus

Torque recommended 30 Ncm



Straight Abutment:

ICA130C. Straight Abutment Ø 4.5 H 1.5 JDIcon Plus
 ICSA4520C. Straight Abutment Ø 4.5 H 2.0 JDIcon Plus
 ICSA4520NEC. Straight Abutment Non Engaging Ø 4.5 H 2.0 JDIcon Plus
 ICSA4540C. Straight Abutment Ø 4.5 H 4.0 JDIcon Plus
 ICSA4540NEC. Straight Abutment Non Engaging Ø 4.5 H 4.0 JDIcon Plus
 ICSA5020C. Straight Abutment Ø 5.0 H 2.0 JDIcon Plus
 ICSA5020NEC. Straight Abutment Non Engaging Ø 5.0 H 2.0 JDIcon Plus
 ICSA5040C. Straight Abutment Ø 5.0 H 4.0 JDIcon Plus
 ICSA5040NEC. Straight Abutment Non Engaging Ø 5.0 H 4.0 JDIcon Plus
 ICSA6020C. Straight Abutment Ø 6.0 H 2.0 JDIcon Plus
 ICSA6040C. Straight Abutment Ø 6.0 H 4.0 JDIcon Plus

Torque recommended 30 Ncm



Torque recommended 30 Ncm



GP Abutment:

ICGP40C. GP Abutment Ø 4.0 JDIcon Plus
 ICGP50C. GP Abutment Ø 5.0 JDIcon Plus
 ICGP60C. GP Abutment Ø 6.0 JDIcon Plus
 IC15GPAEC. GP Abutment 15° JDIcon Plus
 IC25GPAEC. GP Abutment 25° JDIcon Plus

Torque recommended 30 Ncm



Anatomic Abutment:

IC15A15C. Anatomic Abutment Angulated 15° H 1.5 JDIcon Plus
 IC15A30C. Anatomic Abutment Angulated 15° H 3.0 JDIcon Plus
 IC25A15C. Anatomic Abutment Angulated 25° H 1.5 JDIcon Plus
 IC25A30C. Anatomic Abutment Angulated 25° H 3.0 JDIcon Plus


Torque recommended 30 Ncm



Cobalt-Chrome Abutment:

ICCCEC. Cobalt-Chrome Abutment Engaging JDIcon Plus
 ICCCNEC. Cobalt-Chrome Abutment Non Engaging JDIcon Plus
 EVCACCNEC. Cobalt-Chrome Conical Abutment Non Engaging JDEvolution

Torque recommended 30 Ncm



15 Ncm

Prosthetic Screw:

ICS.	Prosthetic Screw JDIcon Plus
ICSA.	Prosthetic Screw Angulated JDIcon Plus

Torque recommended 30 Ncm



Extra Abutment:

ICEXA5520C.	Straight Abutment Extra Ø 5.5 H 2.0 JDIcon Plus
ICEXA5540C.	Straight Abutment Extra Ø 5.5 H 4.0 JDIcon Plus
ICEXTIBC.	TiBase Extra Engaging Ø4.25 H 0.5 C 4.7 JDIcon Plus
ICEXTIBNEC.	TiBase TiBase Extra Non Engaging Ø4.25 H 0.5 C 4.7 JDIcon Plus
ICEXTIB15C.	TiBase Extra Engaging Ø4.25 H 1.5 C 4.7 JDIcon Plus
ICEXTIB15NEC.	TiBase Extra Non Engaging Ø4.25 H 1.5 C 4.7 JDIcon Plus
ICEXTIB30C.	TiBase Extra Engaging Ø4.25 H 3.0 C 4.7 JDIcon Plus
ICEXTIB30NEC.	TiBase Extra Non Engaging Ø4.25 H 3.0 C 4.7 JDIcon Plus



Torque recommended 30 Ncm

Octa Abutment:

ICOA15.	Octa Abutment H 1.5 JDIcon Plus
ICOA30.	Octa Abutment H 3.0 JDIcon Plus
ICOA40.	Octa Abutment H 4.0 JDIcon Plus
ICOA50.	Octa Abutment H 5.0 JDIcon Plus
ICOA60.	Octa Abutment H 6.0 JDIcon Plus
ICOAHC.	Healing Cap Octa Abutment JDIcon Plus
ICOAHC54.	Healing Cap Octa Abutment D 5.0 H 4.0 JDIcon Plus
ICOAICOTC.	Impression Coping Open Tray for Octa Abutment JDIcon Plus
ICOAICOTEC.	Impression Coping Open Tray Engaging for Octa Abutment JDIcon Plus
ICOAR.	Octa Abutment Replica JDIcon Plus
ICOAPS.	Prosthetic Screw Octa Abutment JDIcon Plus
ICOAPSA.	Prosthetic Screw Angulated Octa Abutment JDIcon Plus
ICOAWANEC.	Wax-Up Abutment Non Engaging Octa Abutment JDIcon Plus
ICOATANEC.	Temporary Abutment Non Engaging Octa Abutment JDIcon Plus
ICOATAEC.	Temporary Abutment Engaging Octa Abutment JDIcon Plus
ICOAITC.	Interface CAD CAM Octa Abutment JDIcon Plus (Ø4.45 C7.3)
ICOAITEC.	Interface CAD CAM Engaging Octa Abutment JDIcon Plus (Ø4.45 C7.3)
ICOATIBC.	TiBase Octa Abutment JDIcon Plus (Ø4.45 C5.0)
ICOATIBEC.	TiBase Octa Abutment Engaging JDIcon Plus (Ø4.45 C5.0)
ICOASBCEC.	ScanBody Octa Abutment JDIcon Plus
ICOASBCEEC.	ScanBody Engaging Octa Abutment JDIcon Plus
ICOARC.	Octa Abutment Replica CAD CAM JDIcon Plus

Torque recommended 30 Ncm



Torque recommended 30 Ncm



Torque recommended 30 Ncm



Torque recommended 30 Ncm

Conical Abutment:

ICCA15C.	Conical Abutment H 1.5 JDIcon Plus
ICCA30C.	Conical Abutment H 3.0 JDIcon Plus
ICCA40C.	Conical Abutment H 4.0 JDIcon Plus
ICCA1725C.	Conical Abutment Angulated 17° H 2.5 JDIcon Plus
ICCA1735C.	Conical Abutment Angulated 17° H 3.5 JDIcon Plus
ICCA3025C.	Conical Abutment Angulated 30° H 2.5 JDIcon Plus
ICCA3035C.	Conical Abutment Angulated 30° H 3.5 JDIcon Plus
ICCA1740NC.	Conical Abutment Slim Plus 17° H 4.0 JDIcon Plus
ICCA1750NC.	Conical Abutment Slim Plus 17° H 5.0 JDIcon Plus
ICCA3050NC.	Conical Abutment Slim Plus 30° H 5.0 JDIcon Plus
ICCA3060NC.	Conical Abutment Slim Plus 30° H 6.0 JDIcon Plus
ICCASA.	Conical Abutment Angulated Screw JDIcon Plus
EVCAPS.	Prosthetic Screw Conical Abutment JDEvolution
EVCAPSA.	Prosthetic Screw Angulated for Conical Abutment JDEvolution
EVCAPSN:	Prosthetic Screw Conical Abutment Direct N*
EVCAPDNA.	Prosthetic Screw for Angulated Channel Conical Abutment Direct N
EVCAICOTEC.	Conical Abutment Impression Coping Open Tray Engaging JDEvolution
EVCAICOTC.	Conical Abutment Impression Coping Open Tray JDEvolution
EVCAICOTLC.	Conical Abutment Impression Coping Open Tray Long JDEvolution
EVCAICOT02.	Screw for Conical Abutment Impression Coping Open Tray JDEvolution
EVCAICOT04.	Screw for Conical Abutment Impression Coping Open Tray Long JDEvolution
EVCAICCTC.	Conical Abutment Impression Coping Closed Tray
EVCAHC.	Conical Abutment Healing Cap JDEvolution
EVCAHCL.	Conical Abutment Healing Cap H 6.0 JDEvolution
EVCAHC9.	Conical Abutment Healing Cap H 9.0 JDEvolution
EVCAHCB.	Conical Abutment Healing Cap Peek JDEvolution

Torque recommended 30 Ncm



Torque recommended 30 Ncm




Torque recommended 30 Ncm



Torque recommended 30 Ncm



Torque recommended 15 Ncm

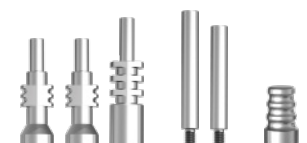

Torque recommended 15 Ncm



EVCAGPAEC
EVCAGPANEC
EVCATANEWSC
EVCATANEC
EVCATANEWC
EVCWANEC
EVCAAR

GP Abutment Engaging for Conical Abutment JDEvolution
GP Abutment Non Engaging for Conical Abutment JDEvolution
Temporary Abutment Non Engaging Conical Abutment Smooth for Welding JDEvolution
Temporary Abutment Non Engaging Conical Abutment JDEvolution
Temporary Abutment Non Engaging Conical Abutment for Welding JDEvolution
Wax-Up Abutment Non Engaging for Conical Abutment
Conical Abutment Replica

*for screw use JDEvolution Plus prosthetic screwdriver




TiBase, JDSanBody and Implant Replica CAD CAM:

ICSBCEC.
EVCASBCEC
EVCASBCEEC
EVCASBCECSC:
JDSCGIOSE
JDSCGIOS
JDSCGIOSR
ICHBSB53.
ICHBSB55.
ICHBSB57.
ICTIBC.
ICTIBNEC.
ICTIB15C.
ICTIB15NEC.
ICTIB30C.
ICTIB30NEC.
ICTIBNC.
ICTIBNENC.
ICTIB10NC.
ICTIB10NENC.
ICTIB15NC.
ICTIB15NENC.
ICTIB20NC.
ICTIB20NENC.
ICTIB30NC.
ICTIB30NENC.
ICTIB40NC.
ICTIB40NENC.
ICTIBNAC.
ICTIBNENAC.
ICTIB15NAC.
ICTIB15NENAC.
ICTIB30NAC.
ICTIB30NENAC.
EVCAITEC
EVA139C
EVCAITC
EVCATIBC
EVCAITAC
EVS110
EVS111
EVS112
ICANC.
EVCAARCN
ICPMNC.

ScanBody Engaging JDIcon Plus
ScanBody Conical Abutment JDEvolution
ScanBody Engaging Conical Abutment
On Top ScanBody Conical Abutment JDEvolution Plus*
ScanBody Full Arch Tracer Hexagonal
ScanBody Full Arch Tracer
ScanBody Rectangular Full Arch Tracer
On Top ScanBody Engaging Ø 5.0 H 3.0 JDIcon Plus
On Top ScanBody Engaging Ø 5.0 H 5.0 JDIcon Plus
On Top ScanBody Engaging Ø 5.0 H 7.0 JDIcon Plus
TiBase Engaging Ø4.25 H 0.5 C 4.7 JDIcon Plus
TiBase Non Engaging Ø4.25 H 0.5 C 4.7 JDIcon Plus
TiBase Engaging Ø4.25 H 1.5 C 4.7 JDIcon Plus
TiBase Non Engaging Ø4.25 H 1.5 C 4.7 JDIcon Plus
TiBase Engaging Ø4.25 H 3.0 C 4.7 JDIcon Plus
TiBase Non Engaging Ø4.25 H 3.0 C 4.7 JDIcon Plus
TiBase Long engaging Ø4.4 H 0.5 C 7.7 JDIcon Plus
TiBase Long Non Engaging Ø4.4 H 0.5 C 7.7 JDIcon Plus
TiBase New Engaging Ø4.4 H 1.0 C 7.7 JDIcon Plus
TiBase New Non Engaging Ø4.4 H 1.0 C 7.7 JDIcon Plus
TiBase Long Engaging Ø4.4 H 1.5 C 7.7 JDIcon Plus
TiBase Long Non Engaging Ø4.4 H 1.5 C 7.7 JDIcon Plus
TiBase New Engaging Ø4.4 H 2.0 C 7.7 JDIcon Plus
TiBase New Non Engaging Ø4.4 H 2.0 C 7.7 JDIcon Plus
TiBase Long Engaging Ø4.4 H 3.0 C 7.7 JDIcon Plus
TiBase Long Non Engaging Ø4.4 H 3.0 C 7.7 JDIcon Plus
TiBase Long Engaging Ø4.4 H 4.0 C 7.7 JDIcon Plus
TiBase Long Non Engaging Ø4.4 H 4.0 C 7.7 JDIcon Plus
TiBase New Engaging Ø4.4 H 0.5 C 7.7 for Angulated Channel JDIcon Plus
TiBase New Non Engaging Ø4.4 H 0.5 C 7.7 for Angulated Channel JDIcon Plus
TiBase New Engaging Ø4.4 H 1.5 C 7.7 for Angulated Channel JDIcon Plus
TiBase New Non Engaging Ø4.4 H 1.5 C 7.7 for Angulated Channel JDIcon Plus
TiBase New Engaging Ø4.4 H 3.0 C 7.7 for Angulated Channel JDIcon Plus
TiBase New Non Engaging Ø4.4 H 3.0 C 7.7 for Angulated Channel JDIcon Plus
Interface CAD CAM for Conical Abutment Engaging JDEvolution (H 7.5)
TiBase Engaging for Conical Abutment (H 5.0)
Interface CAD CAM for Conical Abutment Non Engaging JDEvolution (H 7.3)
TiBase for Conical Abutment JDEvolution (H 5.0)
Interface CAD CAM Non Engaging for Conical Abutment Angulated Channel (H 7.7)
Prosthetic Screw Conical Abutment Direct
Prosthetic Screw Conical Abutment Direct Long
Prosthetic Screw for Angulated Channel Conical Abutment Direct
Implant Replica CAD CAM JDIcon Plus
Conical Abutment Replica CAD CAM New
Pre-milled Abutment Blank JDIcon Plus

*for screw use JDEvolution Plus prosthetic screwdriver

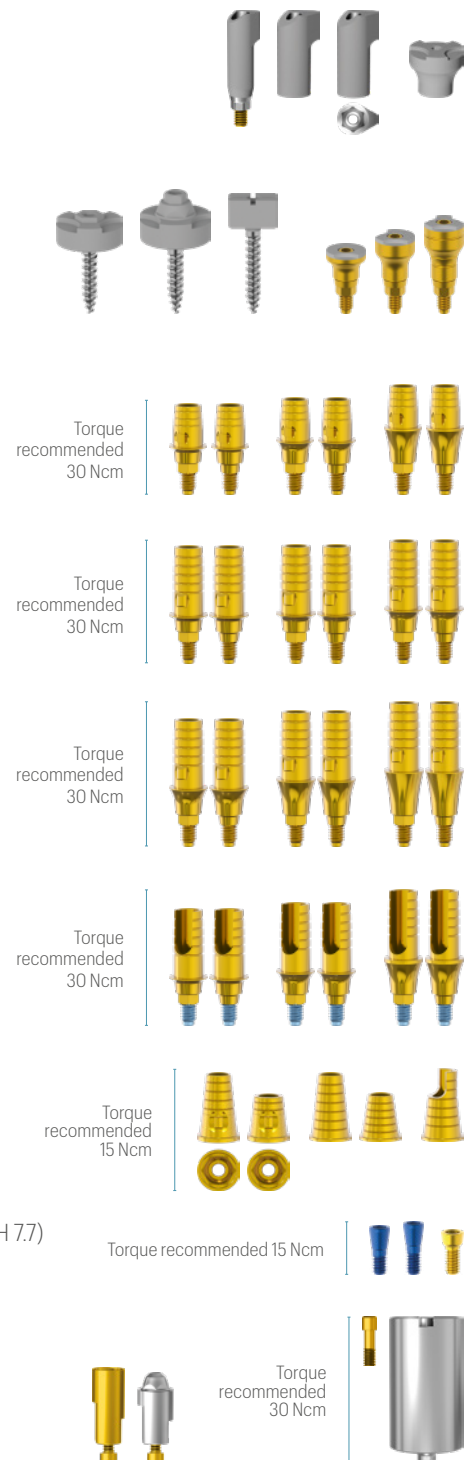

Conical Abutments Mini:

ICCA15MIC.
ICCA30MIC.
ICCA40MIC.
EVCAHCMIC
EVCAHCLMIC
EVCAITMIC
EVCAITMIEC
EVCATBMIC
EVCATBMIEC

Conical Straight Abutment MINI H 1.5 JDIcon Plus
Conical Straight Abutment MINI H 3.0 JDIcon Plus
Conical Straight Abutment MINI H 4.0 JDIcon Plus
Conical Abutment MINI Healing Cap
Conical Abutment MINI Healing Cap H 6.0
Interface CAD CAM Non Engaging H 7.0 for Conical Abutment MINI
Interface CAD CAM Engaging H 7.0 for Conical Abutment MINI
Interface CAD CAM Non Engaging H 5.0 for Conical Abutment MINI
Interface CAD CAM Engaging H 5.0 for Conical Abutment* MINI



EVCATANEMIC	Temporary Abutment Non Engaging Conical Abutment MINI
EVCAICOTMIC	Conical Abutment MINI Impression Coping Open Tray
EVCAICOTMIEC	Conical Abutment MINI Impression Coping Engaging Open Tray
EVCAARM1	Conical Abutment MINI Replica
EVCAARMIC	Conical Abutment MINI Replica CAD CAM
EVCASBCEMIC	ScanBody Conical Abutment MINI
EVCASBCEMIEC	ScanBody Engaging Conical Abutment MINI
EVCASBCESMIC:	On Top ScanBody Conical Abutment MINI



Conometric Abutment:

ICCP05C.	Conometric Abutment Straight H 0.5 JDICon Plus
ICCP10C.	Conometric Abutment Straight H 1.0 JDICon Plus
ICCP20C.	Conometric Abutment Straight H 2.0 JDICon Plus
ICCP30C.	Conometric Abutment Straight H 3.0 JDICon Plus
ICCP40C.	Conometric Abutment Straight H 4.0 JDICon Plus
IC7CP20C.	7.5° Angulated Conometric Abutment H 2.0 JDICon Plus
IC7CP20NEC.	7.5° Angulated Conometric Abutment Non Engaging H 2.0 JDICon Plus
IC15CP20C.	15° Angulated Conometric Abutment H 2.0 JDICon Plus
IC15CP20NEC.	15° Angulated Conometric Abutment Non Engaging H 2.0 JDICon Plus
IC22CP20C.	22.5° Angulated Conometric Abutment H 2.0 JDICon Plus
IC22CP20NEC.	22.5° Angulated Conometric Abutment Non Engaging H 2.0 JDICon Plus
ICA300C.	30° Angulated Conometric Abutment H 2.0 JDICon Plus
IC30CP20NEC.	30° Angulated Conometric Abutment Non Engaging H 2.0 JDICon Plus
EVA130C:	Cap With Pin for Intraoral Welding
EVA131C:	Cap for Partial or Full-Arch Fixed Prosthesis
EVA132C:	Anti-Rotation Cap for Single Element
EVCPIIC	Conometric Abutment Impression Coping PEEK
EVCPAN	Conometric Abutment Replica

Torque recommended 30 Ncm



Torque recommended 30 Ncm



Ball Abutment:

ICBA15.	Ball Abutment H 1.5 JDICon Plus
ICBA30.	Ball Abutment H 3.0 JDICon Plus
ICBA50.	Ball Abutment H 5.0 JDICon Plus
EVBA	Ball Abutment Replica
EVBAHC	Ball Abutment Elastic Retention Cap w/ Container
EVBAN	Ball Abutment Retention Cap


Torque recommended 30 Ncm



Emi Abutment:

ICEMI15.	Emi Abutment H 1.5 JDICon Plus
ICEMI30.	Emi Abutment H 3.0 JDICon Plus
ICEMI50.	Emi Abutment H 5.0 JDICon Plus
EVEMISCK	Smart cap attachment Emi Abutment
EVEMIHC	Emi Abutment Elastic Retention Cap w/ Container
EVEMIN	Emi Abutment Elastic Retention Cap (1.2 kg)
EVEMIH	Emi Abutment Container
EVEMIIC	Emi Abutment Plastic Impression Coping
EVEMIICS	Emi Abutment Steel Impression Coping
EVEMINT	Emi Abutment White Retention Cap (1.8 kg)
EVEMINY	Emi Abutment Yellow Retention Cap (0.6 kg)
EVEMINP	Emi Abutment Purple Retention Cap (2.5 kg)
EVEMINB	Emi Abutment Retention Cap for Laboratory
EVEMIA	Emi Abutment Replica
EVEMIEIT	Extractor-insertion Tool For Caps

Torque recommended 30 Ncm

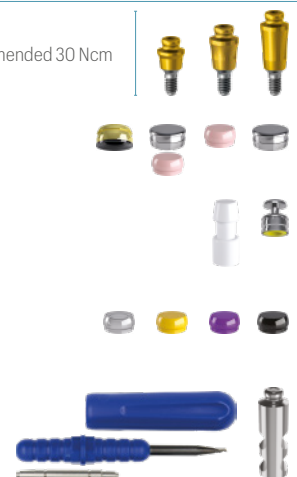

Implant replica:

ICAN.	Implant Replica JDICon Plus
-------	-----------------------------



Bone Mill:

ICBM5C.	Bone Mill Ø 5.0 and Guide JDICon Plus
ICBM6C.	Bone Mill Ø 6.0 and Guide JDICon Plus
ICBMG.	Bone Mill Guide JDICon Plus



Short Drills:

JDDICS4	Short Drill Ø 4mm L 6 JDIcon Plus
JDDICS4D	Short Drill Ø 4mm L 6 Dense Bone JDIcon Plus
JDDICS5	Short Drill Ø 5mm L 6 JDIcon Plus



Direction indicators:

JDDI	Direction Indicator
JDDIS	Direction Indicator Short
JDDI17	Direction Indicator 17°
JDDI30	Direction Indicator 30°
JDDI45	Direction Indicator 45°



Implant and Prosthetic Drivers:

ICID.	Implant Driver JDIcon Plus
ICIDL.	Implant Driver Long JDIcon Plus
ICIDPT.	Implant Driver Long JDIcon Plus PT

EVSDPF15	Prosthetic Driver for JDTorque L 15
EVSDPF20	Prosthetic Driver for JDTorque L 20
EVSDPF25	Prosthetic Driver for JDTorque L 25
EVSDPF35	Prosthetic Driver for JDTorque L 35
EVSDPF60	Prosthetic Driver for JDTorque L 60
ICOASDF.	Octa Abutment Driver for JDTorque
ICOASDFL.	Octa Abutment Driver Long for JDTorque
EVSDCAF	Conical Abutment Driver for JDTorque


EVSDP20	Prosthetic Driver L 20
EVSDP25	Prosthetic Driver L 25
EVSDP30	Prosthetic Driver L 30
JDPD103	Prosthetic Driver for Surgical Driver
EVSDCA	Conical Abutment Driver
JDPD108	Octa Abutment Driver

EVSDPF25A	Angulated Screw Driver for JDTorque L 25
EVSDPF30A	Angulated Screw Driver for JDTorque L 30
EVSDPF25AV	Angulated Screw Driver for Conical Abutment Direct JDTorque L 25
EVSDPF30AV	Angulated Screw Driver for Conical Abutment Direct JDTorque L 30
EVSDP32AV	Screw Driver for Conical Abutment Direct EVS112 (Straight Channel)

ICATR27.	Abutment Removal Driver L 27 JDIcon Plus
ICATR34.	Abutment Removal Driver L 34 JDIcon Plus

EVSUD	Surgical Driver JDEvolution
JDG	JDGuide
ICGMC.	Implant Mounter for JDIcon Plus
ICGMLC.	Implant Mounter Long for JDIcon Plus
JDID105	Conical Abutment Aligning Instrument JDIcon Plus

JDSPR	Dental Implant Depth Probe
JDNPR	26 mm Depth Probe JDNasal

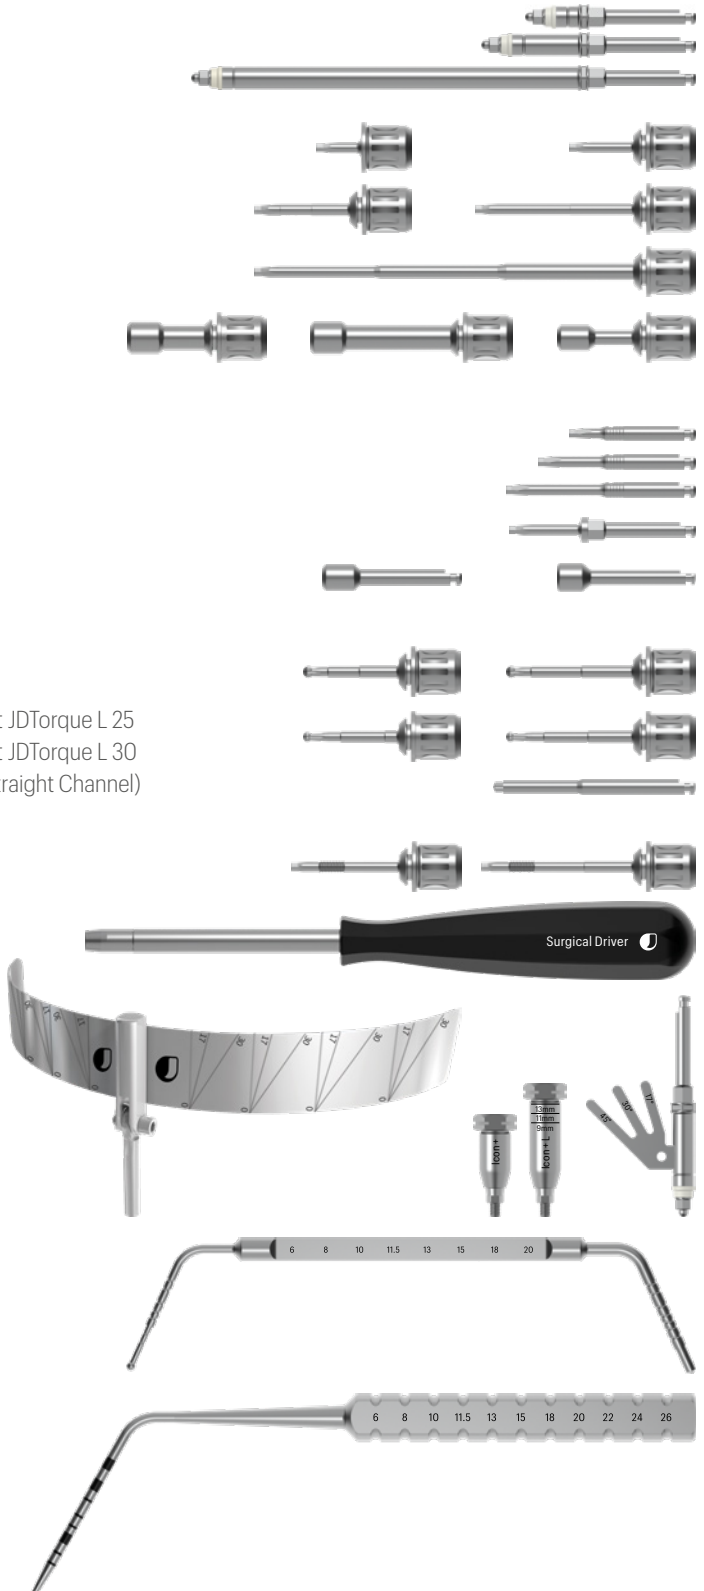


DRILLING PROTOCOLS

It is recommended to adhere to the indications of the following drilling sequence to ensure optimal primary stability of the implant

	HEALED BONE		POST EXTRACTIVE BONE		 Short Implant L 6mm JDIcon Plus insertion in maxilla	
IMPLANT DIAMETER	SOFT BONE	MEDIUM-DENSE BONE	SOFT BONE	MEDIUM-DENSE BONE		
site preparation in maxilla						
Ø 3,7	2,0 2,4 2,8 up to the 1 st laser mark L 6mm	2,0 2,4 2,8 3,2 up to the 1 st laser mark L 6mm	2,0 2,4 2,8 at the entrance	2,0 2,4 2,8 at the entrance	 Short Implant L 6mm JDIcon Plus insertion in mandible	
Ø 4,3	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 up to the 1 st laser mark L 6-8mm 3,6 at the entrance	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance		
Ø 5,0	2,0 2,4 2,8 3,2 3,6 up to the 1 st laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 st laser mark L 6mm 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1 st laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1 st laser mark L 6mm		
site preparation in mandible					 Short Implant L 6mm JDIcon Plus insertion in maxilla	
Ø 3,7	2,0 2,4 2,8 3,2 at the entrance 3,6 at the entrance up to the 1 st laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 st laser mark L 6mm	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance		
Ø 4,3	2,0 2,4 2,8 3,2 3,6 at the entrance 4,0 at the entrance up to the 2 nd laser mark L 8mm	2,0 2,4 2,8 3,2 3,6 4,0 up to the 2 nd laser mark L 8mm 4,4 up to the 1 st laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance		
Ø 5,0	2,0 2,4 2,8 3,2 3,6 4,0 4,4 at the entrance 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	- Start the osteotomy with standard twist drill Ø 2.0mm, Ø 2.4mm and Ø 2.8mm - Complete with the Ø 4mm L 6 JDIcon Plus drill JDDICS4D	
Ø 5,0	2,0 2,4 2,8 3,2 3,6 4,0 4,4 at the entrance 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	- Start the osteotomy with standard twist drill Ø 2.0mm, Ø 2.4mm and Ø 2.8mm - Complete with the Ø 5mm L 6 JDIcon Plus drill JDDICS5	

Note: all measurements in mm

Note: For the surgical procedure for the insertion of JDIcon Plus PT and JDIcon Plus LE fixtures, please refer to the surgical manual available at www.jdentalcare.com

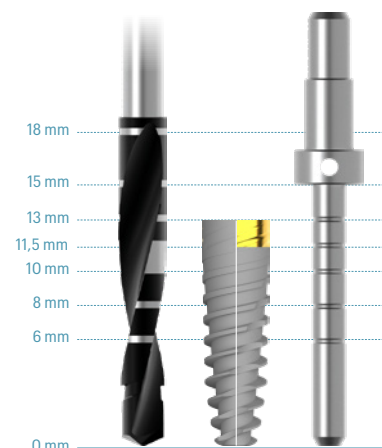

NOTE

Handwriting practice lines consisting of 28 horizontal dotted lines.



JDENTALCARE

www.jdentalcare.com

JDentalCare, the JDentalCare logo and other trademarks mentioned in this document are, excluding specifically mentioned exceptions, trademarks property of JDentalCare.

The images of the products represented in this brochure are not necessarily to scale.

Note: Not all products manufactured by JDentalCare and represented in this brochure have been regulatory cleared/released for sale in all countries and/or have been licensed in accordance with FDA Rules and Regulations.

For more information about current product assortment and availability, please contact your local JDentalCare distributor. For prescription only.

Caution: Federal (US) law restricts this device to sale by or on the other for a licensed dentist. See instructions for use for more information such as indications, warnings, precaution and contraindications.

ICPCAT
REV.47 of 2026-07-21